


**GORE® VIABAHN®**

Endoprosthesis  
with PROPATEN Bioactive Surface\*

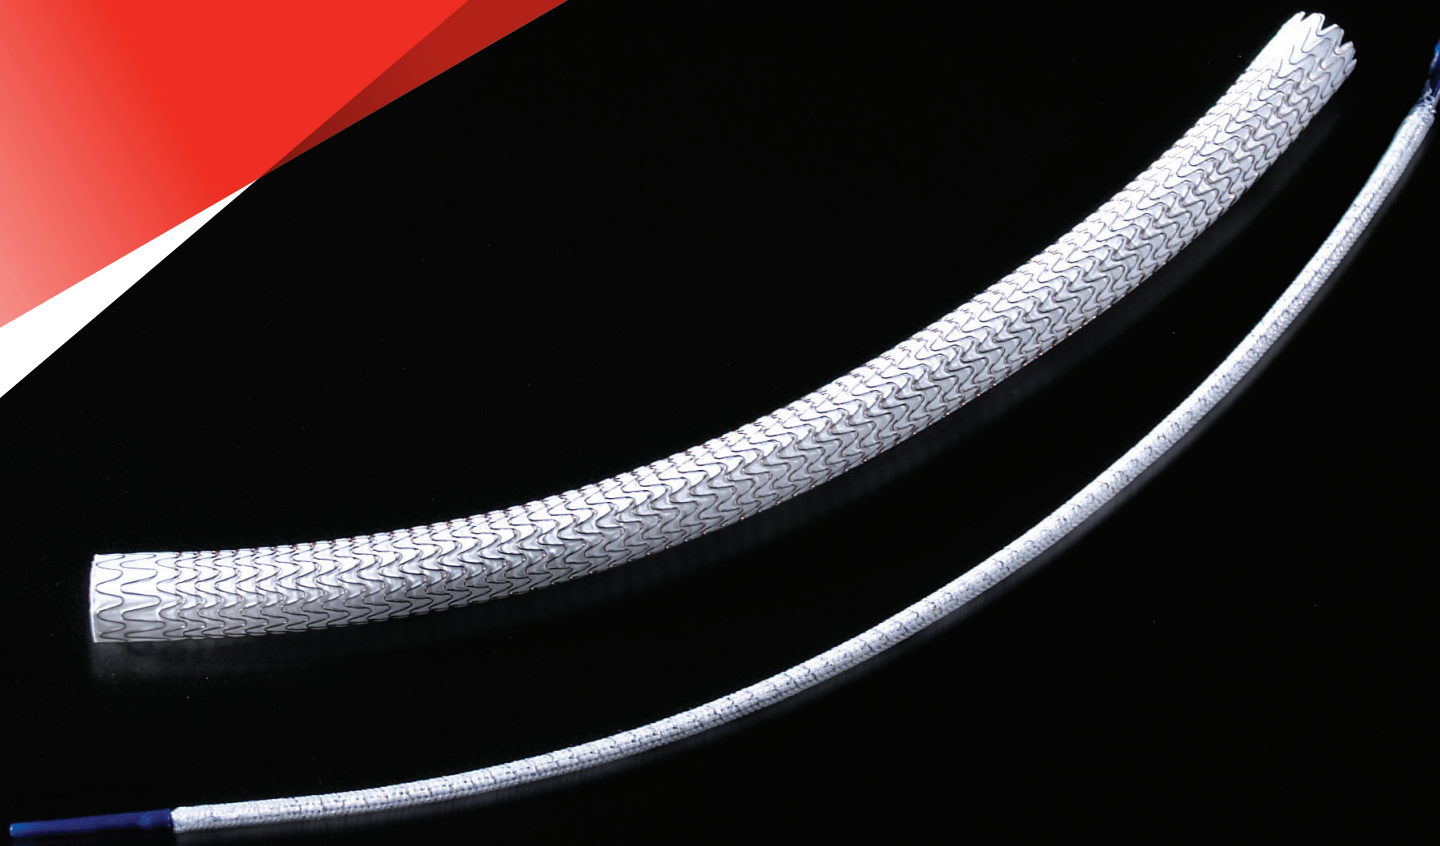

# CONFIGURATIONS

\*As used by Gore, PROPATEN Bioactive Surface refers to Gore's proprietary CBAS Heparin Surface.

*Together, improving life*



# Catalogue listings

## .035" Guidewire

Catalogue number	Endoprosthesis labeled diameter* (mm)	Endoprosthesis length* (cm)	Catheter length† (cm)	Recommended vessel diameter† (mm)	Device profile <sup>§</sup> (Fr)	Recommended balloon diameter for device touch-up <sup>  </sup> (mm)
PAH050202K	5	2.5	120	4.0 – 4.7	7	5
PAH050502K	5	5	120	4.0 – 4.7	7	5
PAH051002K	5	10	120	4.0 – 4.7	7	5
PAH051502K	5	15	120	4.0 – 4.7	7	5
PAH052502K	5	25	120	4.0 – 4.7	7	5
PAH060202K	6	2.5	120	4.8 – 5.5	7	6
PAH060502K	6	5	120	4.8 – 5.5	7	6
PAH061002K	6	10	120	4.8 – 5.5	7	6
PAH061502K	6	15	120	4.8 – 5.5	7	6
PAH062502K	6	25	120	4.8 – 5.5	7	6
PAH070202K	7	2.5	120	5.6 – 6.5	8	7
PAH070502K	7	5	120	5.6 – 6.5	8	7
PAH071002K	7	10	120	5.6 – 6.5	8	7
PAH071502K	7	15	120	5.6 – 6.5	8	7
PAH072502K	7	25	120	5.6 – 6.5	8	7
PAH080202K	8	2.5	120	6.6 – 7.5	8	8
PAH080502K	8	5	120	6.6 – 7.5	8	8
PAH081002K	8	10	120	6.6 – 7.5	8	8
PAH081502K	8	15	120	6.6 – 7.5	8	8
PAH082502K	8	25	120	6.6 – 7.5	8 <sup>†</sup>	8

Catalogue number	Endoprosthesis labeled diameter* (mm)	Endoprosthesis length* (cm)	Catheter length† (cm)	Recommended vessel diameter‡ (mm)	Device profile§ (Fr)	Recommended balloon diameter for device touch-up¶ (mm)
PAH090502K	9	5	120	7.6 – 8.5	9	9
PAH091002K	9	10	120	7.6 – 8.5	9	9
PAH091502K	9	15	120	7.6 – 8.5	9	9
PAH100502K	10	5	120	8.6 – 9.5	11§	10
PAH101002K	10	10	120	8.6 – 9.5	11§	10
PAH101502K	10	15	120	8.6 – 9.5	11§	10
PAH110502K	11	5	120	9.6 – 10.5	11	12
PAH111002K	11	10	120	9.6 – 10.5	11	12
PAH130502K	13	5	120	10.6 – 12.0	12	14
PAH131002K	13	10	120	10.6 – 12.0	12	14

\* Labeled device diameters and lengths are nominal.

† Ensure the guidewire is the appropriate size (see *Instructions for Use*) and has a length at least twice that of the delivery catheter.

‡ Recommended endoprosthesis compression within the vessel is approximately 5–20%.

§ The 10 mm diameter device is compatible with the following 10 Fr introducer sheaths: Cordis AVANTI® Sheath Introducer, Boston Scientific SUPER SHEATH Introducer Sheath, B. Braun INTRADYN Tear-Away Introducer Sheath.

¶ For the 11 and 13 mm diameter devices, balloon inflation pressure should not exceed 8 atm.

¶ The 8 mm x 25 cm device is not compatible with the 7 Fr COOK® CHECK-FLO® Introducer.

 Consult Instructions  
for Use  
[eifu.goremedical.com](http://eifu.goremedical.com)

The GORE® VIABAHN® Endoprosthesis with PROPATEN Bioactive Surface is a flexible, self-expanding endoluminal prosthesis for endovascular grafting of peripheral arteries. Refer to *Instructions for Use* at [eifu.goremedical.com](http://eifu.goremedical.com) for a complete description of indications, contraindications, warnings, precautions and adverse events. <sup>Rx</sup> only

Name of product: GORE® VIABAHN® Endoprosthesis with PROPATEN Bioactive Surface

ANVISA registration number: 80067930027

Publication date: May 2021

Classification: IV

Products listed may not be available in all markets.

SUPER SHEATH is a trademark of Boston Scientific. INTRADYN is a trademark of B. Braun Medical, Inc.

COOK, CHECK-FLO, and FLEXOR are trademarks of Cook Medical, Inc. AVANTI is a trademark of Cordis Corporation.

GORE, *Together, improving life*, VIABAHN and designs are trademarks of W. L. Gore & Associates.

© 2021 W. L. Gore & Associates, Inc. 2187214-EN MAY 2021

---

**W. L. Gore & Associates, Inc.**

[goremedical.com](http://goremedical.com)

**Asia Pacific** +65 67332882 **Australia/New Zealand** 1800 680 424 **Europe** 00800 6334 4673

**United States** Flagstaff, AZ 86004 800 437 8181 928 779 2771

