

TRUSTED PERFORMANCE. UNMATCHED VERSATILITY.*


Trusted procedural performance in the treatment of complex aortoiliac occlusive disease (AIOD):

- 100% delivery to target lesion with no device dislodgement.¹
- 100% restoration of lumen diameter.¹

Sustained clinical effectiveness through 5 years:

- 89.5% primary patency and 96.1% primary assisted patency per lesion.²
- 89.1% freedom from target lesion revascularization (fTLR) per subject.²
- 100% of patients improved ≥ 1 Rutherford category vs. baseline.²

This physician-initiated study enrolled 59 patients from 3 participating centers with patients followed out to 5 years and beyond.

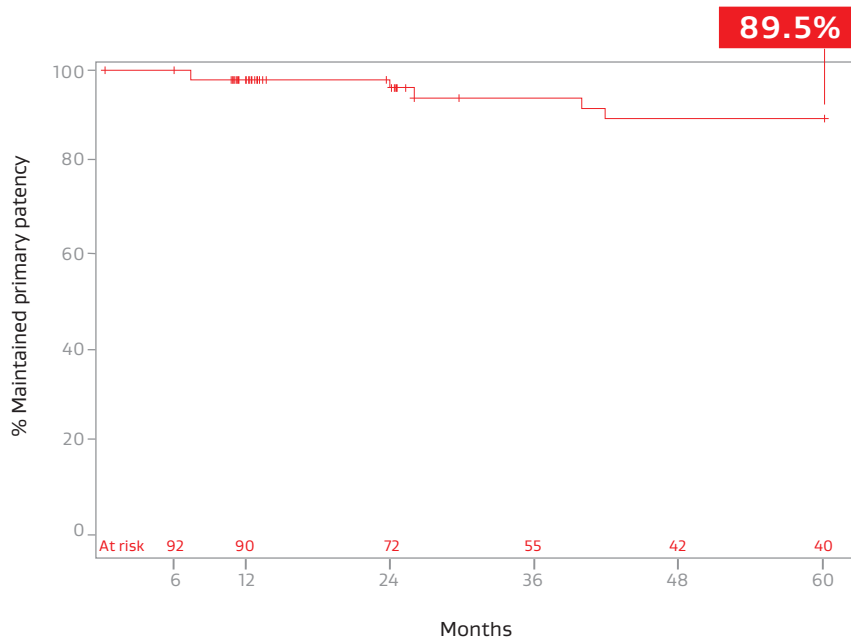

Kaplan-Meier graph of primary patency with number of lesions at risk

* Across indication inclusivity and configuration breadth/capability of balloon expandable covered stents. Procedural outcomes based on usage of legacy GORE® VIABAHN® VBX Balloon Expandable Endoprosthesis (BXA catalogue numbers).

Same endoprosthesis and trusted performance, now with greater versatility.

- The most 6 Fr compatible configurations of any balloon expandable covered stent.³⁻⁵
- A lower delivery profile enables a 1 Fr reduction on most sizes.

Stent labeled/ nominal diameter (mm)	Stent length (mm)	Legacy profile (Fr)	Current profile (Fr)
5	15/19/29/39/59/79	7	6
6	15/19/29/39/59/79	7	6
7	15/19/29/39/59/79	7	6
8	29/39/59	7	7
8	79	8	7
8L	29/39	7	7
8L	59/79	8	8
9	29/39/59/79	8	7
10	29/39/59/79	8	8
11	29/39/59/79	8	8


NOW
6Fr
compatible
**GREAT
VERSATILITY**

All configurations available in .035" over-the-wire 80 cm and 135 cm catheter lengths.

References

1. Bismuth J, Gray BH, Holden A, Metzger C, Panneton J; VBX FLEX Study Investigators. Pivotal study of a next-generation balloon-expandable stent-graft for treatment of iliac occlusive disease. *Journal of Endovascular Therapy* 2017;24(5):629-637.
2. Holden A, Takele E, Hill A, et al. Long-term follow-up of subjects with iliac occlusive disease treated with the Viabahn VBX Balloon-Expandable Endoprosthesis. *Journal of Endovascular Therapy*. In press.
3. GORE® VIABAHN® VBX Balloon Expandable Endoprosthesis [Instructions for Use]. Flagstaff, AZ: W. L. Gore & Associates, Inc; 2023. MD169334.
4. LIFESTREAM® Balloon Expandable Vascular Covered Stent [Instructions for Use]. Tempe, AZ: Bard Peripheral Vascular, Inc; 2019. BAW1345700 Rev. 5 06/19.
5. iCast covered stent system [Instructions for Use]. Merrimack, NH: Atrium Medical Corporation; 2023. AW009603-EN Rev 11.

 Consult Instructions
for Use
eifu.goremedical.com

INDICATIONS FOR USE IN THE U.S.: The GORE® VIABAHN® VBX Balloon Expandable Endoprosthesis is indicated for the treatment of de novo or restenotic lesions found in iliac arteries with reference vessel diameters ranging from 5 mm–13 mm and lesion lengths up to 110 mm, including lesions at the aortic bifurcation. The GORE® VIABAHN® VBX Balloon Expandable Endoprosthesis is also indicated for use with thoracoabdominal and pararenal branched devices indicated with the GORE® VIABAHN® VBX Balloon Expandable Endoprosthesis as a branch component. **CONTRAINDICATIONS:** Do not use the GORE® VIABAHN® VBX Balloon Expandable Endoprosthesis in patients with known hypersensitivity to heparin, including those patients who have had a previous incident of Heparin-Induced Thrombocytopenia (HIT) type II. Refer to *Instructions for Use* at eifu.goremedical.com for a complete description of all applicable indications, warnings, precautions and contraindications for the markets where this product is available. 

* Not applicable to reduced profile GORE® VIABAHN® VBX Balloon Expandable Endoprosthesis (BxB catalogue numbers).

Products listed may not be available in all markets.

GORE, *Together, improving life*, VBX, VIABAHN and designs are trademarks of W. L. Gore & Associates.
© 2024 W. L. Gore & Associates, Inc. 24LP1147-EN01 SEPTEMBER 2024

W. L. Gore & Associates, Inc.
goremedical.com

Asia Pacific +65 67332882 Australia / New Zealand 1800 680 424 Europe 00800 6334 4673
United States Flagstaff, AZ 86004 800 437 8181 928 779 2771

